


3077981005

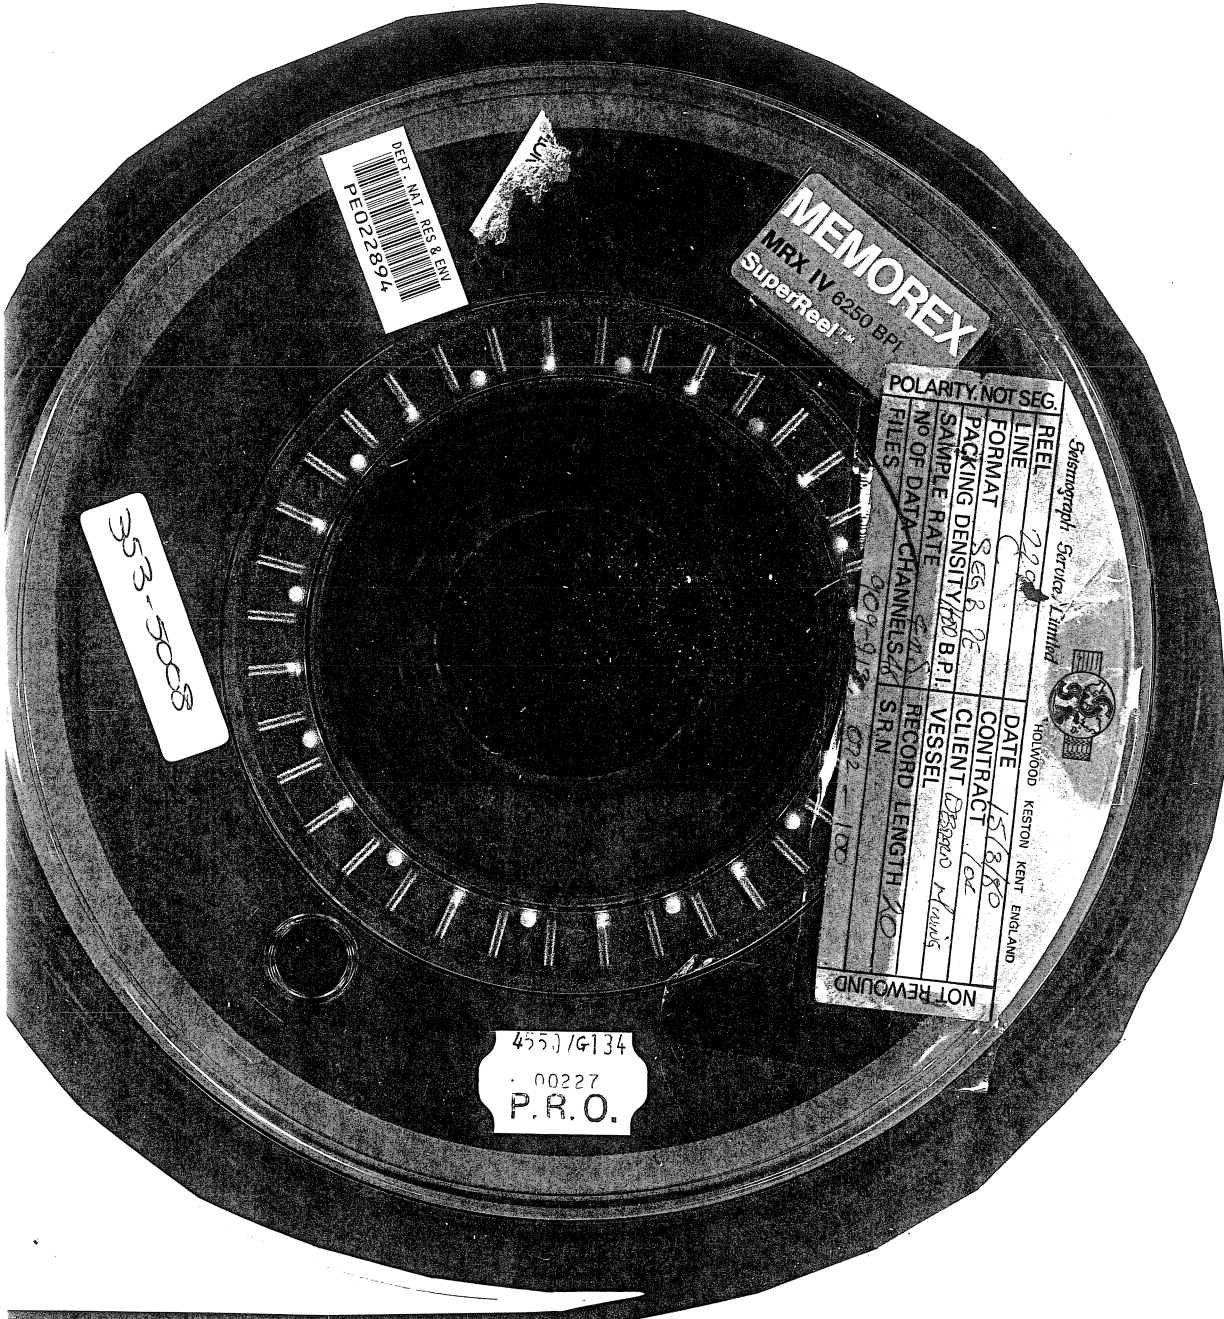

DEPT. INT. SEC. & EX. INT.
PEO22894

MEMOREX
MRX IV 6250 BPI
SuperReel™

353-5008

POLARITY NOT SEC.	
REEL LINE	228
FORMAT	SES & 2e
PACKING DENSITY	400 BPI
SAMPLE RATE	2700
No OF DATA CHANNELS	2
FILES	909-918
DATE	15/8/80
CONTRACT	for
CLIENT	Dr. David Lewis
VESSEL	
RECORD LENGTH	20
S.R.N.	022-100

Stenograph Service Limited
HOLWOOD KESTON KENT ENGLAND

4550/G134
. 00227
P.R.O.